

Fig. 1

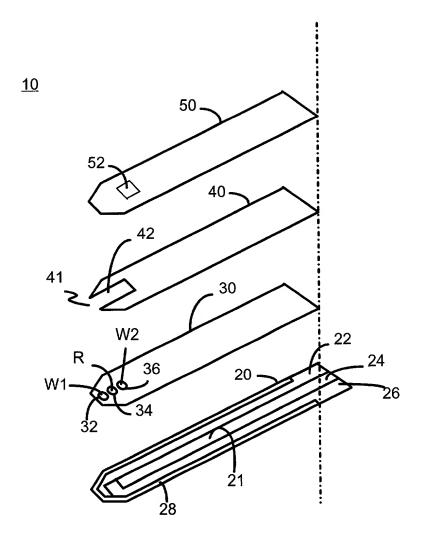


Fig. 2

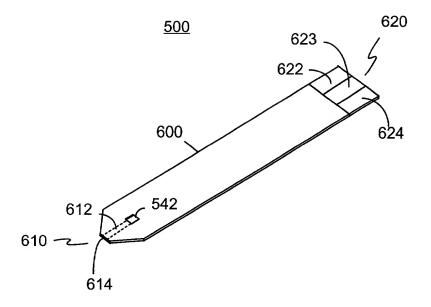


Fig. 3

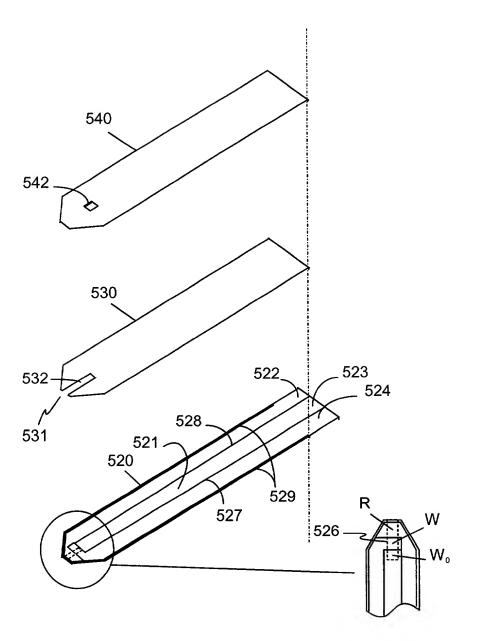


Fig. 4

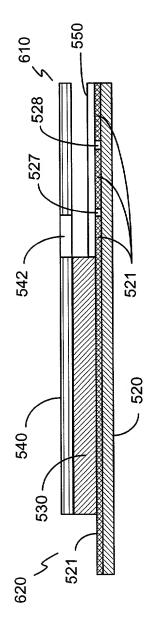


Fig. 5

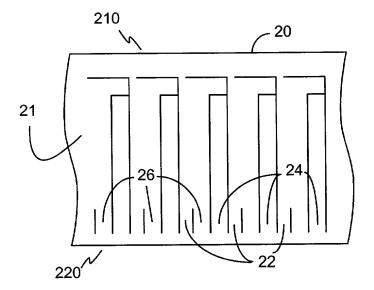


Fig. 6A

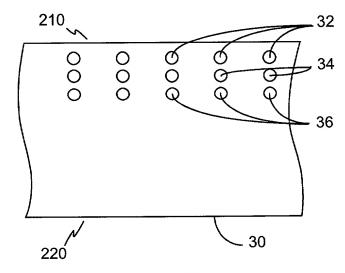
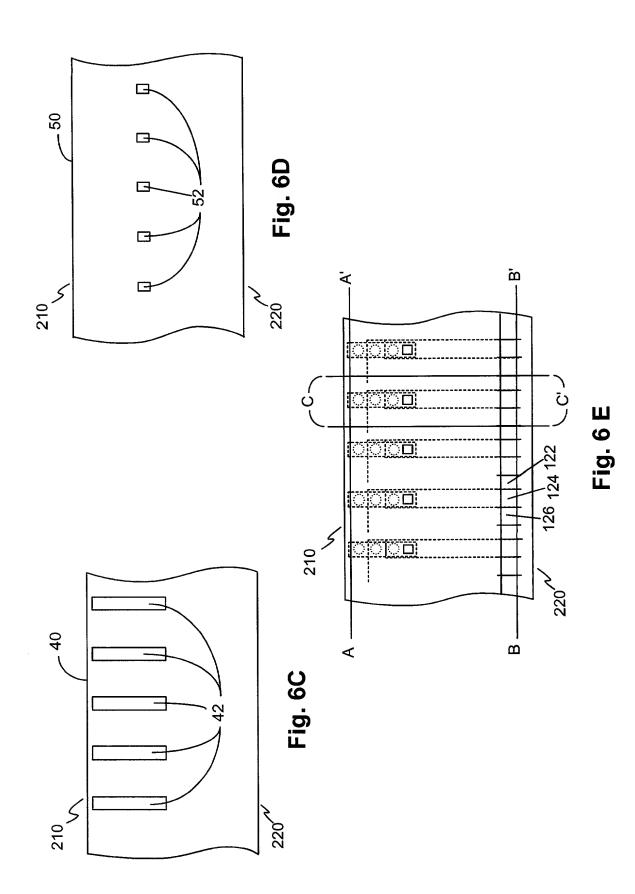


Fig. 6B



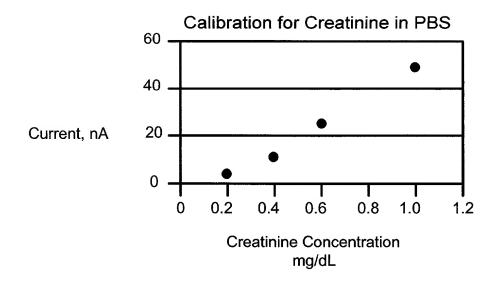


Fig. 7A

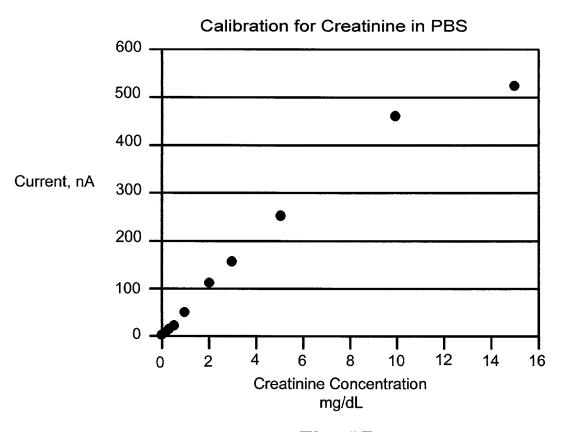
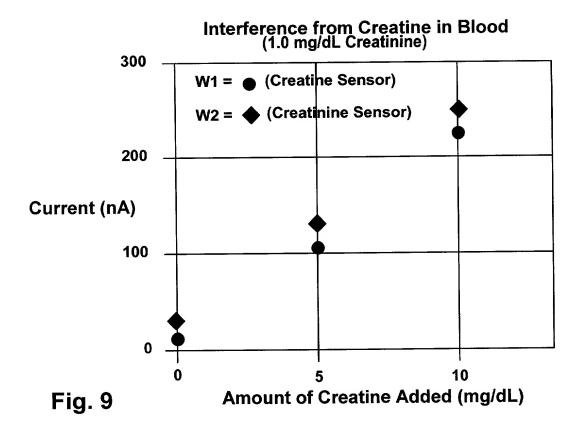



Fig. 7B


Calibration for Creatinine in Blood 500 -400 -Current, nA 15 Spiked Creatinine Concentration

Fig. 8

mg/dL



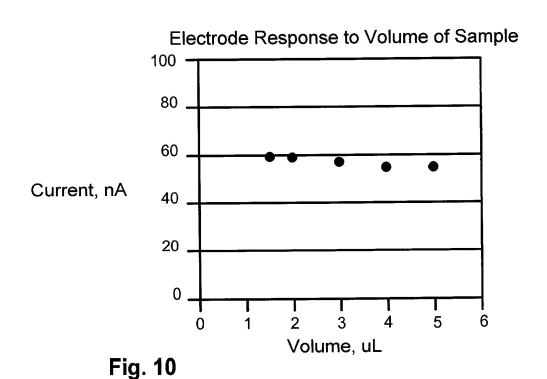

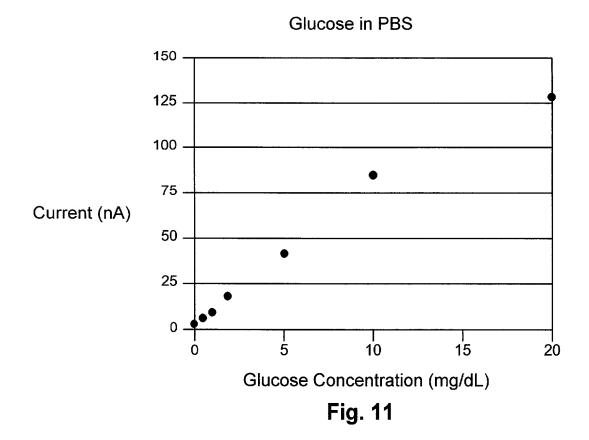

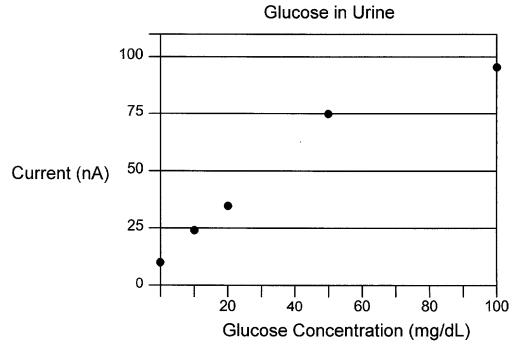


Fig. 12

Fig. 13

